

GRUPPO PIAZZETTA S.P.A TEST REPORT

SCOPE OF WORK

EPA EMISSIONS TESTING FOR MODEL MONIA 2.0

REPORT NUMBER

103455277MID-002

TEST DATE(S)

02/21/19

ISSUE DATE **[REVISED DATE]**

02/26/19


PAGES

23

DOCUMENT CONTROL NUMBER

GFT-OP-10c (05/10/17)

© 2017 INTERTEK

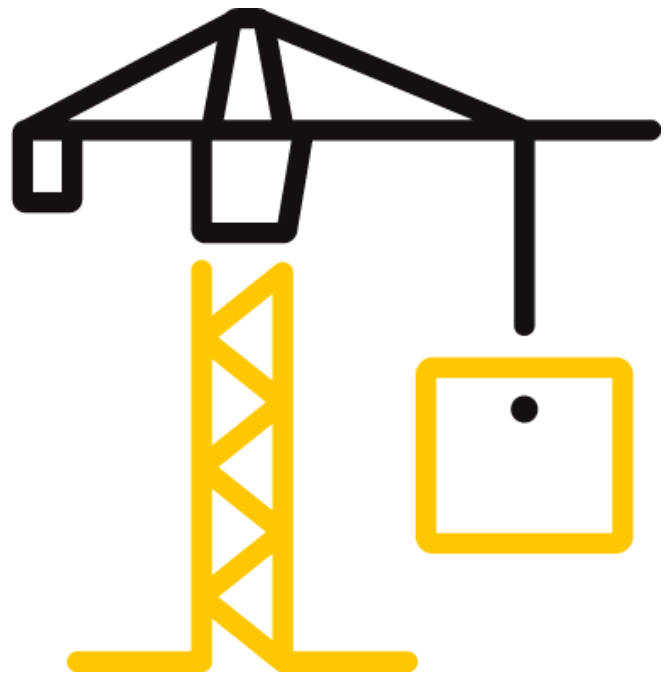

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

REPORT ISSUED TO

GRUPPO PIAZZETTA S.P.A

Via Montello, 22

Casella D'Asolo, TV 31011

Italy

SECTION 1

SCOPE

Intertek Building & Construction (B&C) was contracted by Gruppo Piazzetta S.p.A, Via Montello, 22, Casella D'Asolo, TV 31011, Italy to perform testing in accordance with EPA 40 CFR Part 60 "Standards of Performance for New Residential Wood Heaters, New Residential Hydronic Heaters and Forced-Air Furnaces", ASTM E2515-11- Standard Test Method for Determination of Particulate Matter Emissions Collected by a Dilution Tunnel, ASTM E2779-10 - Standard Test Method for Determining Particulate Matter Emissions from Pellet Heaters, and CSA B415.1-10 - Performance Testing of Solid-Fuel-Burning Heating Appliances on their Model Monia 2.0, Pellet Fuel Room Heater. Results obtained are tested values and were secured by using the designated test method(s). Testing was conducted at Intertek test facility in Middleton, WI.

This report does not constitute certification of this product nor an opinion or endorsement by this laboratory.

SECTION 2

SUMMARY OF TEST RESULTS



The appliance tests resulted in the following performance:

Particulate Emissions: 0.820 g/hr

Carbon Monoxide Emissions: 0.00 g/min

Heating Efficiency: 82.4 % (Higher Heating Value Basis)

For INTERTEK B&C:

COMPLETED BY:	Ken Slater	REVIEWED BY:	Brian Ziegler
TITLE:	Associate Engineer – Hearth	TITLE:	Technical Team Leader - Hearth
SIGNATURE:	 Ken Slater	SIGNATURE:	
DATE:	02/26/19	DATE:	02/26/19

aaa:bbb

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

SECTION 3

TEST METHOD(S)

The specimen was evaluated in accordance with the following:

EPA 40 CFR Part 60-2015 - Standards of Performance for New Residential Wood Heaters, New Residential Hydronic Heaters and Forced-Air Furnaces

ASTM E2515-2011 - Standard Test Method for Determination of Particulate Matter Emissions Collected by a Dilution Tunnel

ASTM E2779-2010 - Standard Test Method for Determining Particulate Matter Emissions from Pellet Heaters

CSA B415.1-2010 - Performance Testing of Solid-Fuel-Burning Heating Appliances

SECTION 4

MATERIAL SOURCE

A sample was submitted to Intertek directly from the client. The sample was not independently selected for testing. The test unit was received at Intertek in Middleton, WI on 2/13/19 and was shipped via the client. The unit was assigned sample ID # MID1902131240-001. The unit was inspected upon receipt and found to be in good condition. The unit was set up following the manufacturer's instructions without difficulty.

Following assembly, the unit was placed on the test stand. Prior to beginning the emissions tests, the unit was operated for a minimum of 10 hours at high-to-medium burn rates to break in the stove. This break-in period was conducted by Intertek staff and a copy of the data is included in the final report. The unit was found to be operating satisfactory during this break-in. The 10 plus hours of pre-burning were conducted from 02/14/19 through 02/15/19. The fuel used for the break-in process was wood pellets.

Following the pre-burn break-in process the unit was allowed to cool and ash and residue was removed from the firebox. The unit's chimney system and laboratory dilution tunnels were cleaned using standard wire brush chimney cleaning equipment. On 02/20/19 the unit was set-up for testing.

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

**SECTION 5
EQUIPMENT**

Equipment	INV Number	Calibration Due	MU
Platform Scale	008	4/10/19	+ 27g
Balance	713	4/10/19	+ 0.47mg
Data Logger	986	4/10/19	+ 0.33°F
Scale	1134	4/10/19	+ 27g
Timer	1212	4/4/19	+ 0.3 sec
Timer	1213	4/4/19	+ 0.3 sec
Flow Meter	1413	7/18/19	+ 17mL/min
Flow Meter	1414	7/18/19	+ 17mL/min
Barometer	1420	4/12/19	+ 0.24°F, 1.7%RH, 0.011 in Hg
DGM	1210	6/27/19	+ 0.00284 ft ³

**SECTION 6
LIST OF OFFICIAL OBSERVERS**

NAME	COMPANY
Ken Slater	Intertek B&C
Denis De Marchi	Gruppo Piazzetta S.p.A

**SECTION 7
TEST PROCEDURE**

On 02/20/19 and 02/21/19, the unit was tested for EPA emissions. For pellet stoves, the test was conducted in accordance with ASTM E2779-10. The fuel used for the test run was premium-Grade Pellets (Marthwood).

The applicable EPA regulatory limits are:

Step 1 – 2015 – 4.5 grams per hour.

Step 2 – 2020 – 2.0 grams per hour.

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

TEST SET-UP DESCRIPTION

A 3" horizontal flue is connected by a 90° elbow and adapters to a standard 6" diameter vertical single wall pipe and insulated chimney system was installed to 15' above floor level. The single wall pipe extended to 8 feet above the floor and insulated chimney extended the remaining height.

AIR SUPPLY SYSTEM

Combustion air enters a 2" inlet pipe located on the back of the heater, which is directed to the pellet burn pot. All gases exit through the 3" flue also located at the back of the heater. The exhaust gases are assisted by a combustion blower.

TEST FUEL PROPERTIES

Wood pellets used for the testing were manufactured by Marthwood. The pellets have a measured heating value of 8528 Btu/hr (19836 kJ/kg) and a moisture content of 4.46% on a dry basis and 4.27% on a wet basis.

SAMPLING LOCATIONS

Particulate samples are collected from the dilution tunnel at a point 20 feet from the tunnel entrance. The tunnel has two elbows and two mixing baffles in the system ahead of the sampling section. (See Figure 3.) The sampling section is a continuous 13 foot section of 6 inch diameter pipe straight over its entire length. Tunnel velocity pressure is determined by a standard Pitot tube located 60 inches from the beginning of the sampling section. The dry bulb thermocouple is located six inches downstream from the Pitot tube. Tunnel samplers are located 60 inches downstream of the Pitot tube and 36 inches upstream from the end of this section. (See Figure 1.)

Stack gas samples are collected from the steel chimney section 8 feet ± 6 inches above the scale platform. (See Figure 2.)

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

FIGURE 1 – DILUTION TUNNEL


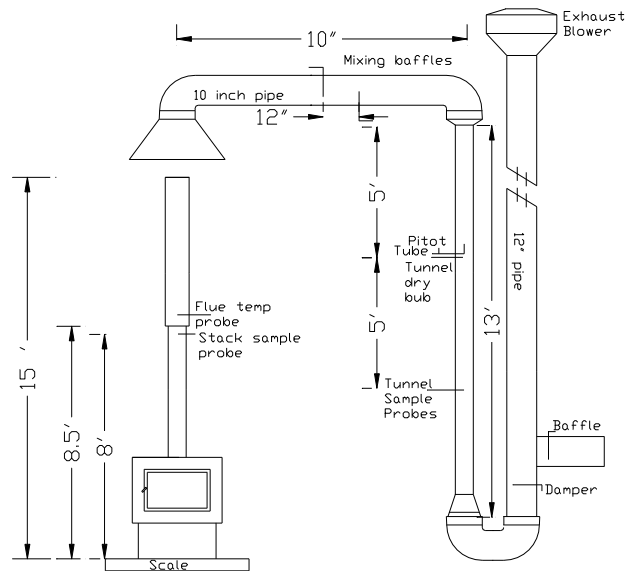


FIGURE 1

FIGURE 2 – STACK GAS SAMPLE TRAIN

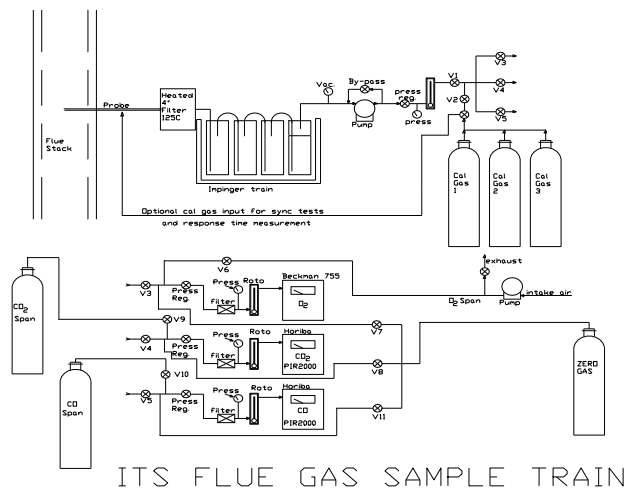

ITS FLUE GAS SAMPLE TRAIN

FIGURE 2

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

FIGURE 3 – DILUTION TUNNEL SAMPLE SYSTEMS

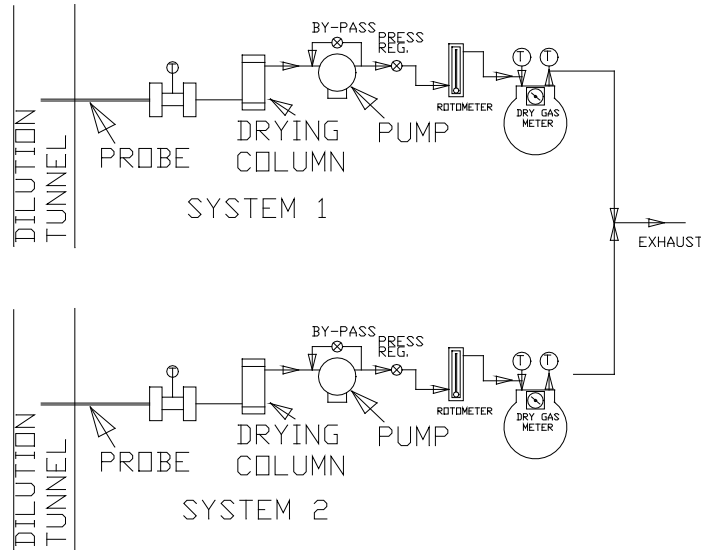


Figure 3

SAMPLING METHODS

PARTICULATE SAMPLING

Particulates were sampled in strict accordance with ASTM E2515-2011. This method uses two identical sampling systems with Gelman A/E 61631 binder free, 47-mm diameter filters. The dryers used in the sample systems are filled with “Drierite” before each test run. In order to measure first-hour emissions rates the a third filter set is prepared at one hour into the test run, the filter sets are changed in one of the two sample trains. The two filter sets used for this train are analyzed individually to determine the first hour and total emissions rate.

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

INSTRUMENT CALIBRATION**DRY GAS METERS**

At the conclusion of each test program the dry gas meters are checked against our standard dry gas meter. Three runs are made on each dry gas meter used during the test program. The average calibration factors obtained are then compared with the six-month calibration factor and, if within 5%, the six-month factor is used to calculate standard volumes. Results of this calibration are contained in Appendix D.

An integral part of the post test calibration procedure is a leak check of the pressure side by plugging the system exhaust and pressurizing the system to 10" W.C. The system is judged to be leak free if it retains the pressure for at least 10 minutes.

The standard dry gas meter is calibrated every 6 months using a Spirometer designed by the EPA Emissions Measurement Branch. The process involves sampling the train operation for 1 cubic foot of volume. With readings made to .001 ft³, the resolution is .1%, giving an accuracy higher than the ±2% required by the standard.

STACK SAMPLE ROTAMETER

The stack sample rotometer is checked by running three tests at each flow rate used during the test program. The flow rate is checked by running the rotometer in series with one of the dry gas meters for 10 minutes with the rotometer at a constant setting. The dry gas meter volume measured is then corrected to standard temperature and pressure conditions. The flow rate determined is then used to calculate actual sampled volumes.

GAS ANALYZERS

The continuous analyzers are zeroed and spanned before each test with appropriate gases. A mid-scale multi-component calibration gas is then analyzed (values are recorded). At the conclusion of a test, the instruments are checked again with zero, span and calibration gases (values are recorded only). The drift in each meter is then calculated and must not exceed 5% of the scale used for the test.

At the conclusion of each unit test program, a three-point calibration check is made. This calibration check must meet accuracy requirements of the applicable standards. Consistent deviations between analyzer readings and calibration gas concentrations are used to correct data before computer processing. Data is also corrected for interferences as prescribed by the instrument manufacturer's instructions.

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

TEST METHOD PROCEDURES**LEAK CHECK PROCEDURES**

Before and after each test, each sample train is tested for leaks. Leakage rates are measured and must not exceed 0.02 CFM or 4% of the sampling rate. Leak checks are performed checking the entire sampling train, not just the dry gas meters. Pre-test and post-test leak checks are conducted with a vacuum of 10 inches of mercury. Vacuum is monitored during each test and the highest vacuum reached is then used for the post test vacuum value. If leakage limits are not met, the test run is rejected. During, these tests the vacuum was typically less than 2 inches of mercury. Thus, leakage rates reported are expected to be much higher than actual leakage during the tests.

TUNNEL VELOCITY/FLOW MEASUREMENT

The tunnel velocity is calculated from a center point Pitot tube signal multiplied by an adjustment factor. This factor is determined by a traverse of the tunnel as prescribed in EPA Method 1. Final tunnel velocities and flow rates are calculated from EPA Method 2, Equation 6.9 and 6.10. (Tunnel cross sectional area is the average from both lines of traverse.)

Pitot tubes are cleaned before each test and leak checks are conducted after each test.

PM SAMPLING PROPORTIONALITY

Proportionality was calculated in accordance with ASTM E2515-11. The data and results are included in Appendix C.

DEVIATIONS FROM STANDARD METHOD:**SECTION 8****TEST CALCULATIONS****WEIGHT OF TEST FUEL BURNED (DRY) – ASTM E2779**

$$M_{Bdb} = (M_{Swb} - M_{Ewb})(100/(100 + FM))$$

where:

FM = average fuel moisture of test fuel, % dry basis,

M_{Swb} = weight of test fuel in hopper at start of test run, wet basis, kg (lb),

M_{Ewb} = weight of test fuel in hopper at end of test run, wet basis, kg (lb), and

M_{Bdb} = weight of test fuel burned during test run, dry basis, kg (lb).

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

WEIGHT OF TEST FUEL BURNED PER TEST SEGMENT (DRY) – ASTM E2779

$$M_{BSidb} = (M_{SSiwb} - M_{ESiwb}) (100/(100 + FM))$$

where:

M_{SSiwb} = weight of test fuel in hopper at start of test run segment i , wet basis, kg (lb),

M_{ESiwb} = weight of test fuel in hopper at end of test run segment i , wet basis, kg (lb),

M_{BSidb} = weight of test fuel burned during test run segment i , dry basis, kg (lb), and

i = test run segments in accordance with 9.4, Table 1.

AVERAGE BURN RATE FOR FULL TEST (DRY) – ASTM E2779

$$BR = 60 M_{Bdb}/\theta$$

where:

BR = average dry burn rate over the full integrated test run, kg/h (lb/h), and

θ = total length of full integrated test run, min.

AVERAGE BURN RATE PER TEST SEGMENT (DRY) – ASTM E2779

$$BR_{Si} = 60 M_{BSidb}/\theta_{Si}$$

where:

BR_{Si} = average dry burn rate over test run segment i , kg/h (lb/h), and

θ_{Si} = total length of test run segment i , min.

AVERAGE EMISSION RATE FOR FULL TEST (g/hr) – ASTM E2779

$$PM_R = 60(E_T/\theta)$$

where:

E_T = total particulate emissions for full integrated test run measured using Test Method **E2515**, g (lb),

θ = total length of test run, min, and

PM_R = average particulate emission rate over the full integrated test run, g/h.

AVERAGE EMISSION FACTOR FOR FULL TEST (g/kg dry) – ASTM E2779

$$PM_F = E_T/M_{Bdb}$$

where:

PM_F = average particulate emission factor over the full integrated test run, g/dry kg of fuel burned.

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

AVERAGE EMISSIONS FOR FULL TEST (g/MJ or lb/MMBtu) – ASTM E2779

$$PM_H = E_T/E_O$$

where:

E_O = average measured overall heat output over the full integrated test run from Annex A1, MJ (MMBTU), and

PM_H = average particulate emissions in accordance with unit of average heat output over the full integrated test run, g/MJ (lb/MMBtu).

NOMENCLATURE FOR ASTM E2515:

A = Cross-sectional area of tunnel m² (ft²).

B_{ws} = Water vapor in the gas stream, proportion by volume (assumed to be 0.02 (2.0 %)).

C_p = Pitot tube coefficient, dimensionless (assigned a value of 0.99).

C_r = Concentration of particulate matter room air, dry basis, corrected to standard conditions, g/dscm (gr/dscf) (mg/dscf).

C_s = Concentration of particulate matter in tunnel gas, dry basis, corrected to standard conditions, g/dscm (gr/dscf) (mg/dscf).

E_T = Total particulate emissions, g.

F_p = Adjustment factor for center of tunnel pitot tube placement.

$$F_p = V_{strav}/V_{scent}$$

K_p = Pitot Tube Constant, $34.97 \frac{m}{sec} \left[\frac{(\frac{g}{g} \cdot mole)(mm\ Hg)}{(K)(mm\ water)} \right]^{\frac{1}{2}}$

or

$$= \text{Pitot Tube Constant, } 85.49 \frac{ft}{sec} \left[\frac{(\frac{lb}{lb} \cdot mole)(in\ Hg)}{(R)(in\ water)} \right]^{\frac{1}{2}}$$

L_a = Maximum acceptable leakage rate for either a pretest or post-test leak-check, equal to 0.0003 m³/min (0.010 cfm) or 4 % of the average sampling rate, whichever is less.

L_p = Leakage rate observed during the post-test leak-check, m³/min (cfm).

m_p = mass of particulate from probe, mg.

m_f = mass of particulate from filters, mg.

m_g = mass of particulate from filter gaskets, mg.

m_r = mass of particulate from the filter, filter gasket, and probe assembly from the room air blank filter holder assembly, mg.

m_n = Total amount of particulate matter collected, mg.

M_s = the dilution tunnel dry gas molecular weight (may be assumed to be 29 g/g mole (lb/lb mole)).

P_{bar} = Barometric pressure at the sampling site, mm Hg (in. Hg).

P_g = Static Pressure in the tunnel (in. water).

P_R = Percent of proportional sampling rate.

P_s = Absolute average gas static pressure in dilution tunnel, mm Hg (in. Hg).

P_{std} = Standard absolute pressure, 760 mm Hg (29.92 in. Hg).

Q_{std} = Average gas flow rate in dilution tunnel.

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

$$Q_{std} = 60 (1 - B_{ws}) V_s A [T_{std} P_s / T_s P_{std}]$$

dscm/min (dscf/min).

T_m = Absolute average dry gas meter temperature, K (R).

T_{mi} = Absolute average dry gas meter temperature during each 10-min interval, i , of the test run.

$$T_{mi} = (T_{mi(b)} + T_{mi(e)})/2$$

where:

$T_{mi(b)}$ = Absolute dry gas meter temperature at the beginning of each 10-min test interval, i , of the test run, K (R), and

$T_{mi(e)}$ = Absolute dry gas meter temperature at the end of each 10-min test interval, i , of the test run, K (R).

T_s = Absolute average gas temperature in the dilution tunnel, K (R).

T_{si} = Absolute average gas temperature in the dilution tunnel during each 10-min interval, i , of the test run, K (R).

$$T_{si} = (T_{si(b)} + T_{m=si(e)})/2$$

where:

$T_{si(b)}$ = Absolute gas temperature in the dilution tunnel at the beginning of each 10-min test interval, i , of the test run, K (R), and

$T_{si(e)}$ = Absolute gas temperature in the dilution tunnel at the end of each 10-min test interval, i , of the test run, K (R).

V_m = Volume of gas sample as measured by dry gas meter, dcm (dcf).

V_{mc} = Volume of gas sampled corrected for the post test leak rate, dcm (dcf).

V_{mi} = Volume of gas sample as measured by dry gas meter during each 10-min interval, i , of the test run, dcm.

$V_{m(std)}$ = Volume of gas sample measured by the dry gas meter, corrected to standard conditions.

$$V_{m(std)} = K_1 V_m Y [(P_{bar} + (\Delta H/13.6))/T_m]$$

where:

K_1 = 0.3855 K/mm Hg for SI units and = 17.64 R/in. Hg for inch-pound units.

$$V_{m(std)} = K_1 V_{mc} Y [(P_{bar} + (\Delta H/13.6))/T_m]$$

where:

V_{mc} = $V_m - (L_p - L_a)u$

V_{mr} = Volume of room air sample as measured by dry gas meter, dcm (dcf), and

$V_{mr(std)}$ = Volume of room air sample measured by the dry gas meter, corrected to standard conditions.

$$V_{m(std)} = K_1 V_{mr} Y [(P_{bar} + (\Delta H/13.6))/T_m]$$

Where:

K_1 = 0.3855 K/mm Hg for SI units and = 17.64 R/in. Hg for inch-pound units, and

V_s = Average gas velocity in the dilution tunnel.

$$V_s = F_p K_p C_p (\sqrt{\Delta P_{avg}})(\sqrt{T_s/P_s M_s})$$

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

- V_{si} = Average gas velocity in dilution tunnel during each 10-min interval, i , of the test run.

$$V_{si} = F_p K_p C_p (\sqrt{\Delta P_i}) (V(T_{si}/P_s M_s))$$
- V_{scent} = Average gas velocity at the center of the dilution tunnel calculated after the Pitot tube traverse.
- V_{strav} = Average gas velocity calculated after the multipoint Pitot traverse.
- Y = Dry gas meter calibration factor.
- ΔH = Average pressure at the outlet of the dry gas meter or the average differential pressure across the orifice meter, if used, mm water (in. water).
- ΔP_{avg} = Average velocity pressure in the dilution tunnel, mm water (in. water).
- ΔP_i = Velocity pressure in the dilution tunnel as measured with the Pitot tube during each 10-min interval, i , of the test run.

$$\Delta P_i = (\Delta P_{i(b)} + \Delta P_{i(e)})/2$$

where:

- $\Delta P_{i(b)}$ = Velocity pressure in the dilution tunnel as measured with the Pitot tube at the beginning of each 10-min interval, i , of the test run, mm water (in. water), and
- $\Delta P_{i(e)}$ = Velocity pressure in the dilution tunnel as measured with the Pitot tube at the end of each 10-min interval, i , of the test run, mm water (in. water).
- θ = Total sampling time, min.
- 10 = ten min, length of first sampling period.
- 13.6 = Specific gravity of mercury.
- 100 = Conversion to percent.

TOTAL PARTICULATE WEIGHT – ASTM E2515

$$M_n = m_p + m_f + m_g$$

PARTICULATE CONCENTRATION – ASTM E2515

$$C_s = K_2(m_n/V_{m(std)}) \text{ g/dscm (g/dscf)}$$

where:

$$K_2 = 0.001 \text{ g/mg}$$

TOTAL PARTICULATE EMISSIONS (g) – ASTM E2515

$$E_T = (C_s - C_r)Q_{std}\theta$$

PROPORTIONAL RATE VARIATION (%) – ASTM E2515

$$PR = [\theta(V_{mi} V_s T_m T_{si}) / (10(V_m V_{si} T_s T_{mi}))] \times 100$$

MEASUREMENT OF UNCERTAINTY – ASTM E2515

$$MU_{weighing} = \sqrt{0.1^2} \cdot X$$

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

GENERAL FORMULA – ASTM E2515

$$uY = \sqrt{((\delta Y/\delta x_1) \times u_1)^2 + \dots + ((\delta Y/\delta x_n) \times u_n)^2}$$

Where:

$\delta Y/\delta x_i$ = Partial derivative of the combining formula with respect to individual measurement x_i ,

u_i = is the uncertainty associated with that measurement.

TOTAL PARTICULATE EMISSIONS – ASTM E2515

$$E_T = (C_s - C_r) Q_{std} \theta$$

where:

C_s = sample filter catch/(sample flow rate x test duration), g/dscf,

C_r = room background filter catch/(sample flow x sampling time), g/dscf,

Q_{std} = average dilution tunnel flow rate, dscf/min, and

θ = sampling time, minutes.

MU OF C_s

$$C_s = F_c/(Q_{sample} \times \theta) = 0.025/(0.25 \times 180) = 0.0005555$$

$$\delta C_s/\delta F_c = 1/Q_{sample} \cdot \theta = 1/0.25 \cdot 180 = 0.0222$$

$$\delta C_s/\delta Q_{sample} = -F_c/Q_{sample}^2 \cdot \theta = -0.025/0.25^2 \cdot 180 = -0.00222$$

$$\delta C_s/\delta \theta = -F_c/Q_{sample} \cdot \theta^2 = -0.025/0.25 \cdot 180^2 = -0.000003$$

$$MU_{C_s} = \sqrt{(0.00027 \cdot 0.0222)^2 + (0.0025 \cdot -0.00222)^2}$$

$$\sqrt{+ (0.1 \cdot -0.000003)^2} = 0.0000091g$$

Thus, C_s would be 0.555 mg/dscf \pm 0.0081 mg/dscf at 95% confidence level.

MU OF C_r

$$C_r = BG_c/(Q_{BG} \times \theta) = 0.002/(0.15 \times 180) = 0.000074$$

$$\delta C_r/\delta BG_c = 1/Q_{BG} \cdot \theta = 1/0.15 \cdot 180 = 0.03704$$

$$\delta C_r/\delta Q_{BG} = -BG_c/Q_{BG}^2 \cdot \theta = -0.002/0.15^2 \cdot 180 = -0.0004938$$

$$\delta C_r/\delta \theta = -BG_c/Q_{BG} \cdot \theta^2 = -0.002/0.15 \cdot 180^2 = -0.0000004$$

$$MU_{C_r} = \sqrt{(0.00027 \cdot 0.03704)^2 + (0.0015 \cdot -0.0004938)^2}$$

$$\sqrt{+ (0.1 \cdot -0.0000004)^2} = 0.00001g$$

Thus, C_r would be 0.074 mg/dscf \pm 0.01 mg/dscf at 95% confidence level.

E_T AND MU_{ET}

$$E_T = (C_s - C_r) Q_{std} \theta = (0.000555 - 0.000074) \times 150 \times 180 = 13.00g$$

$$\delta E_T/\delta C_s = Q_{std} \cdot \theta = 150 \cdot 180 = 27,000$$

$$\delta E_T/\delta C_r = Q_{std} \cdot \theta = 150 \cdot 180 = 27,000$$

$$\delta E_T/\delta Q_{std} = C_s \cdot \theta - C_r \cdot \theta = 0.000555 \cdot 180 - 0.000074 \cdot 180 = 0.08667$$

$$\delta E_T/\delta \theta = C_s \cdot Q_{std} - C_r \cdot Q_{std} = 0.000555 \cdot 180 - 0.000074 \cdot 180 = 0.07222$$

$$MU_{ET} = \sqrt{(27,000 \cdot 0.0000081)^2 + (27,000 \cdot 0.00001)^2 + (0.08667 \cdot 3)^2}$$

$$\sqrt{+ (0.07222 \cdot 0.1)^2} = 0.436$$

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

Thus the result in this example would be:
ET = 13.00g ± 0.44 g at a 95% confidence level.

EFFICIENCY – CSA B415.1

The change in enthalpy of the circulating air shall be calculated using the moisture content and temperature rise of the circulating air, as follows:

$$\Delta h = \Delta t (1.006 + 1.84x)$$

Where:

Δh = change in enthalpy, kJ/kg

Δt = temperature rise, °C

1.006 = specific heat of air, kJ/kg °C

1.84 = specific heat of water vapor, kJ/kg °C

x = humidity ratio, kg/kg

The equivalent duct diameter shall be calculated as follows:

$$ED = 2HW/H+W$$

Where:

ED = equivalent duct diameter

H = duct height, m

W = duct width, m

The air flow velocity shall be calculated as follows:

$$V = F_p \times C_p \times 34.97 \times \sqrt{T/28.56(P_{\text{baro}} + P_s)}$$

where

V = velocity, m/s

F_p = Pitot tube calibration factor determined from vane anemometer measurements

C_p = Pitot factor

= 0.99 for a standard Pitot tube or as determined by calibration for a Type S Pitot tube

34.97 = Pitot tube constant

Note: The Pitot tube constant is determined on the basis of the following units:

$$\text{m/s}[\text{g/g mole (mm Hg)/(K)(mm H}_2\text{O)}]^{0.5}$$

ΔP = velocity pressure, mm H₂O

T = temperature, K

28.56 = molecular weight of air

P_{Baro} = barometric pressure, mm Hg

P_s = duct static pressure, mm Hg

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

The mass flow rate shall be calculated as follows:

$$m = 3600VA\rho$$

where:

m = mass flow rate, kg/h

V = air flow velocity, m/s

3600 = number of seconds per hour

A = duct cross-sectional area, m² ρ = density of air at standard temperature and pressure (use 1.204 kg/m³)

The rate of heat release into the circulating air shall be calculated using the air flow and change in enthalpy, as follows:

$$\Delta e = \Delta h \times m$$

Where:

 Δe = rate of heat release into the circulating air, kJ/h Δh = change in enthalpy of the circulating air, kJ/kg

m = mass air flow rate, kg/h

The heat output over any time interval shall be calculated as the sum of the heat released over each measurement time interval, as follows:

$$E_t = \sum(\Delta e \times i) \text{ for } i = t_1 \text{ to } t_2$$

Where:

 E_t = delivered heat output over any time interval $t_2 - t_1$, kJ

i = time interval for each measurement, h

The average heat output rate over any time interval shall be calculated as follows:

$$e_t = E_t / t$$

where

 e_t = average heat output, kJ/h

t = time interval over which the average output is desired, h

The total heat output during the burn shall be calculated as the sum of all the heat outputs over each time interval, as follows:

$$E_d = \sum(E_t) \text{ for } t = t_0 \text{ to } t_{\text{final}}$$

Where:

 E_d = heat output over a burn, kJ/h (Btu/h) E_t = heat output during each time interval, kJ/h (Btu/h)

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

The efficiency shall be calculated as the total heat output divided by the total energy input, expressed as a percentage as follows:

$$\text{Efficiency, \%} = 100 \times E_d/I$$

Where:

 E_d = total heat output of the appliance over the test period, kJ/kg I = input energy (fuel calorific value as-fired times weight of fuel charge), kJ/kg (Btu/lb)**SECTION 9****TEST SPECIMEN DESCRIPTION**

The model Monia 2.0 Pellet Fuel Room Heater is constructed of sheet steel. The outer dimensions are 19-inches deep, 39-inches high, and 21.25-inches wide. The unit has a door located on the front with a viewing glass.

SECTION 10**TEST RESULTS****DESCRIPTION OF TEST RUNS:**

RUN # 1 (02/20/19): The test for pellet heaters is a continuous test with three separate burn rates. At 7:45am the unit was started and operated for a minimum of 1 hour for the pretest operation. At 9:22am the unit was set to the maximum feed rate (level P4) with a burn rate of 2.09 kg/hr (wet), the scale was tared and a 25-lb weight was added to the scale to determine feed rate of the fuel, and the sampling system was started. At 10:22am, the system #3 sampling filter was changed out and the unit was set to ≤50% feed rate (level P2) with a burn rate of 1.00 kg/hr (wet). At 10:52am client stated that the feed rate parameters were not set correct in the unit and the test was discontinued per client request. This test will not be used.

RUN #2 (02/21/19): The test for pellet heaters is a continuous test with three separate burn rates. At 7:51am the unit was started and operated for a minimum of 1 hour for the pretest operation. At 9:02am the unit was set to the maximum feed rate (level P4) with a burn rate of 2.04 kg/hr (wet), the scale was tared and a 25-lb weight was added to the scale to determine feed rate of the fuel, and the sampling system was started. At 10:02am, the system #3 sampling filter was changed out and the unit was set to ≤50% feed rate (level P2) with a burn rate of 0.97 kg/hr (wet). At 12:02am, the heater was changed to the minimum feed rate (level P1) with a burn rate of 0.71 kg/hr (wet). At 3:02pm, testing was completed. The total burn time was 360 minutes.

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

TABLE 1 – EMISSIONS

RUN#	TEST DATE	BURN RATES (kg/hr)(Dry)		PARTICULATE EMISSION RATE (g/hr)	1 st HOUR EMISSIONS (g)	CO EMISSIONS (g/min)	HEATING EFFICIENCY (%HHV)
2	2/21/19	H*	1.96	0.820	1.185	0.00	82.4
		M*	0.93				
		L*	0.68				
		OA*	0.98				

*Notes: H= High burn rate, M= Medium burn rate, L= low burn rate, OA= overall burn rate.

TABLE 2 – TEST FACILITY CONDITIONS

RUN #	ROOM TEMP BEFORE (°F)	ROOM TEMP AFTER (°F)	BARO PRES BEFORE (in/Hg)	BARO PRES AFTER (in/Hg)	R. H. BEFORE (%)	R. H. AFTER (%)	AIR VEL BEFORE (ft/min)	AIR VEL AFTER (ft/min)
2	69	68	29.01	29.14	21.0	18.0	0	0

TABLE 3 – DILUTION TUNNEL FLOW RATE MEASUREMENTS AND SAMPLING DATA

RUN #	BURN TIME (min)	VELOCITY (ft/sec)	VOLUMETRIC FLOW RATE (dscf/min)	AVG TEMP (°R)	SAMPLE VOLUME (dscf)		PARTICULATE CATCH (mg)	
					1	2	1	2
2	360	22.21	244.03	538.67	83.96	83.85	6.70	7.10

TABLE 4 - DILUTION TUNNEL DUAL TRAIN PRECISION

RUN #	SAMPLE RATIOS		TOTAL EMISSIONS (g)		DEVIATION (%)	DEVIATION (g/kg)
	TRAIN 1	TRAIN 2	TRAIN 1	TRAIN 2		
2	1046.39	1047.79	7.01	7.44	4.32	-0.069

TABLE 5 - GENERAL SUMMARY OF RESULTS

RUN #	BURN RATE (kg/hr)(dry) (OVERALL)	INITIAL DRAFT (in/H ₂ O)	RUN TIME (min)	AVERAGE DRAFT (in/H ₂ O)
2	0.98	0.025	360	0.019

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

TABLE 6 - CSA B415.1 RESULTS

BURN RATE (kg/hr)(dry)	CO EMISSIONS (g/min)	HEATING EFFICIENCY (% HHV)	HEAT OUTPUT (Btu/hr)
HIGH – 1.96	0.00	82.8	30,574
MEDIUM – 0.93	0.00	81.1	14,279
LOW – 0.68	0.00	81.4	10,479
OVERALL – 0.98	0.00	82.4	15,215

SECTION 11**CONCLUSION**

This test demonstrates that the model Monia 2.0 is an affected facility under the definition given in the regulation. The emission rate of 0.820 g/hr meets the EPA requirements for the Step 2 limits.

The results from testing the Monia 2.0 can be extended to similar models Marcella 2.0, Maya 2.0, and Monica 2.0. All models use the same internal components with only external cosmetic differences between each model.

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

SECTION 12 PHOTOGRAPHS

Photo # 1 Emissions test



TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

Photo No. 4

Final security wrap





Total Quality. Assured.

8431 Murphy Drive
Middleton, WI 53562

Telephone: 608-836-4400
Facsimile: 608-831-9279
www.intertek.com/building

TEST REPORT FOR GRUPPO PIAZZETTA S.P.A

Report No.: 103455277MID-002

Date: 02/26/19

SECTION 13
REVISION LOG

REVISION #	DATE	PAGES	REVISION
0	02/26/19	N/A	Original Report Issue